


How to monitor Cushing's

Developed by Ian Ramsey BVSc, PhD, DSAM, Dipl. ECVIM-CA, FHEA, MRCVS, Federico Fracassi DVM, PhD, Dipl. ECVIM-CA, Nadja Sieber-Ruckstuhl PhD, Dr. med. vet, Dipl. ACVIM, Dipl. ECVIM-CA

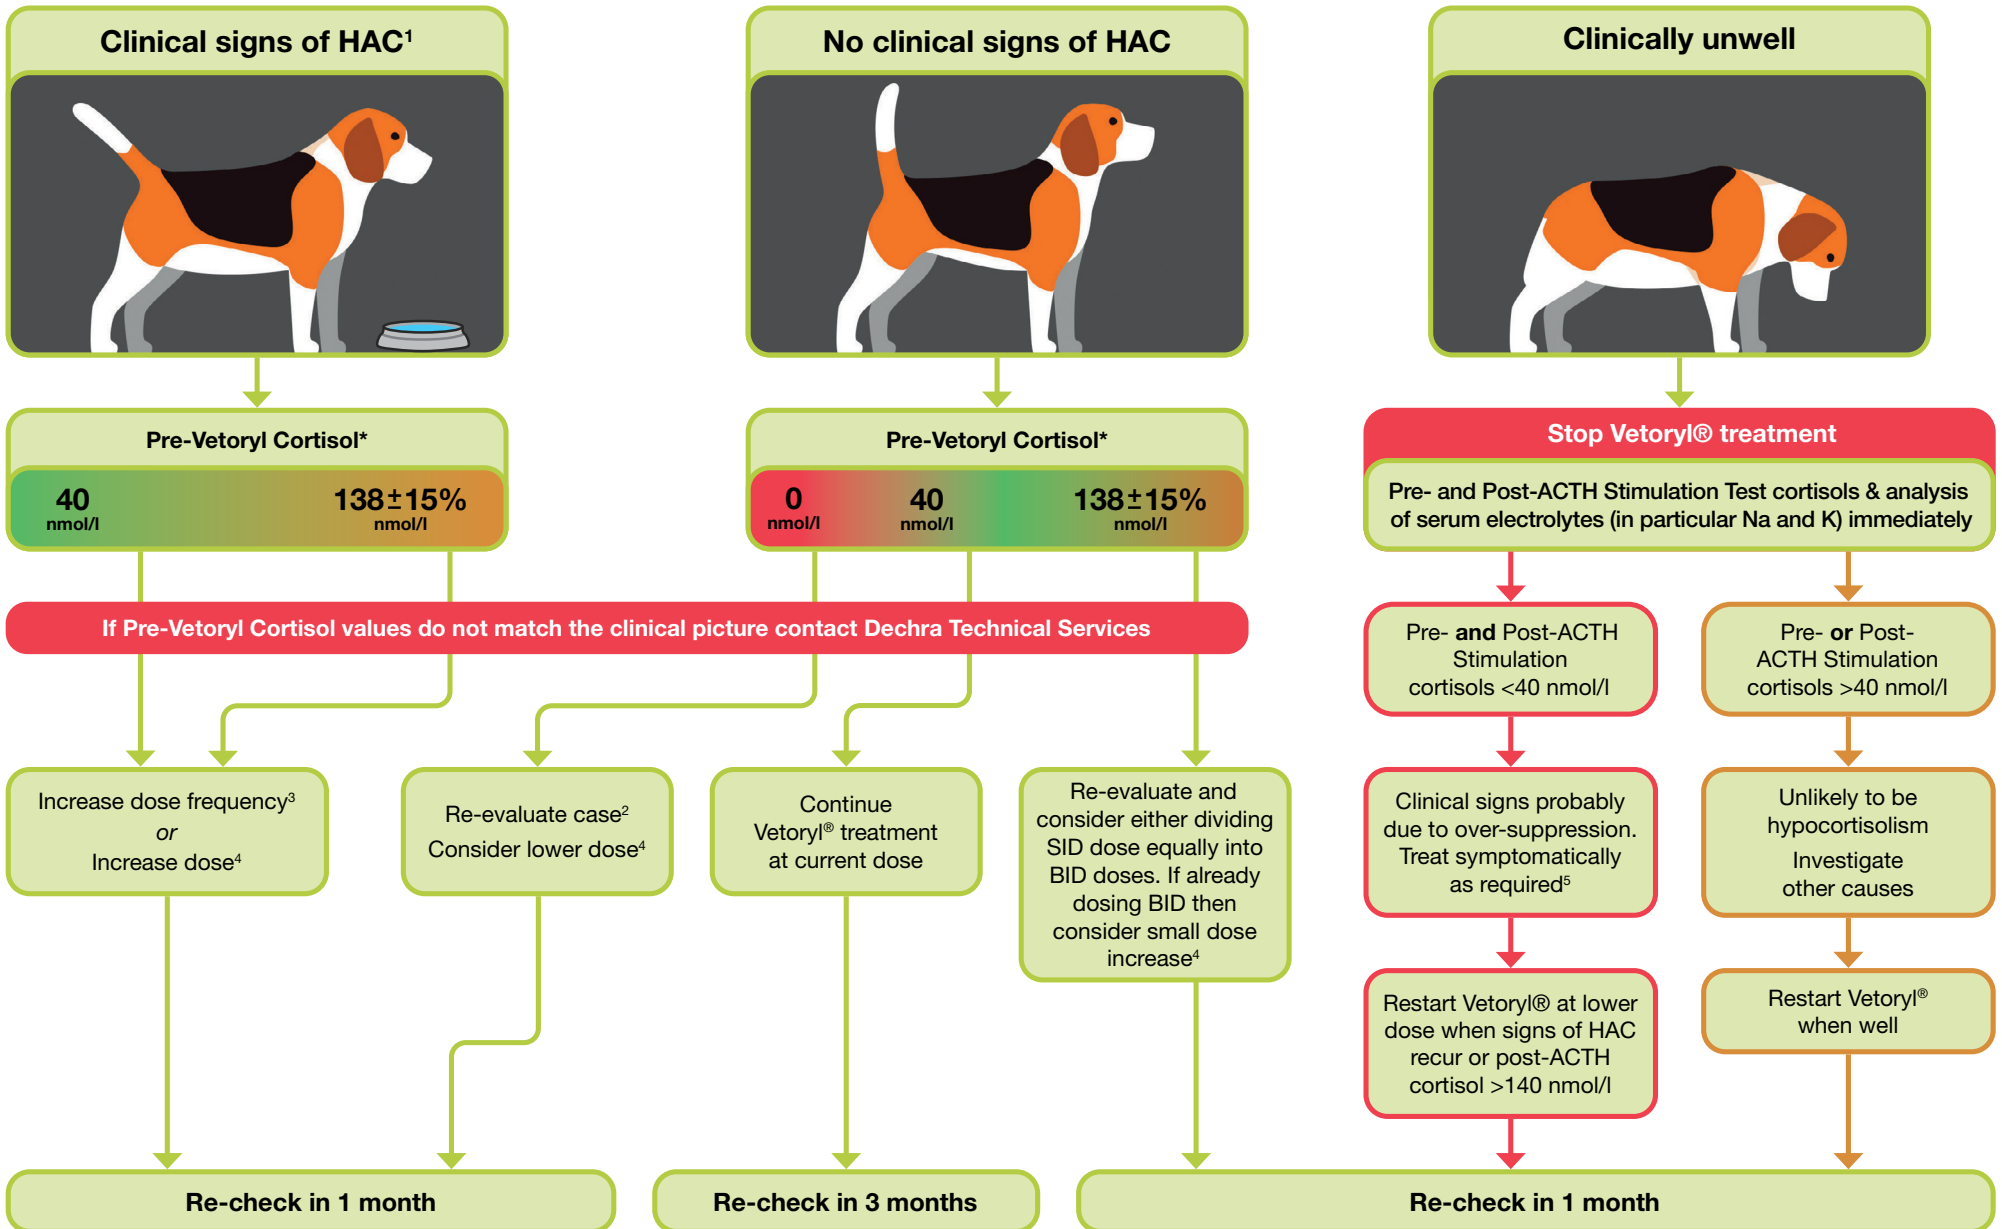

*These figures are based on the use of Siemens IMMULITE 1000/2000 analysers: other analysers may have different thresholds and veterinary surgeons should consult their laboratory if in doubt.